

# VIASURE

## Real Time PCR Detection Kits

by CerTest  
BIOTEC

### SARS-CoV-2

Handbook for the following references/  
Manual para las siguientes referencias:

VIASURE SARS-CoV-2 Real Time PCR Detection Kit 6 x 8-well strips, low profile	VS-NCO206L
VIASURE SARS-CoV-2 Real Time PCR Detection Kit 6 x 8-well strips, high profile	VS-NCO206H
VIASURE SARS-CoV-2 Real Time PCR Detection Kit 12 x 8-well strips, low profile	VS-NCO212L
VIASURE SARS-CoV-2 Real Time PCR Detection Kit 12 x 8-well strips, high profile	VS-NCO212H
VIASURE SARS-CoV-2 Real Time PCR Detection Kit 96-well plate, low profile	VS-NCO213L
VIASURE SARS-CoV-2 Real Time PCR Detection Kit 96-well plate, high profile	VS-NCO213H
VIASURE SARS-CoV-2 Real Time PCR Detection Kit 9 x 4-well strips, Rotor-Gene®	VS-NCO236
VIASURE SARS-CoV-2 Real Time PCR Detection Kit 18 x 4-well strips, Rotor-Gene®	VS-NCO272

For information purposes only



## ENGLISH

### 1. Intended use

VIASURE SARS-CoV-2 Real Time PCR Detection Kit is designed for the specific identification and differentiation of 2019 Novel Coronavirus (SARS-CoV-2) in respiratory samples from patients with signs and symptoms of COVID-19 infection. This test is intended for use as an aid in the diagnosis of SARS-CoV-2 in combination with clinical and epidemiological risk factors. RNA is extracted from respiratory specimens, amplified using RT-PCR and detected using fluorescent reporter dye probes specific for SARS-CoV-2.

### 2. Summary and Explanation

Coronavirus are enveloped non-segmented positive-sense RNA viruses and belong to *Coronaviridae* family. There are six coronavirus species known to cause human diseases. Four viruses (229E, OC43, NL63 and HKU1) cause common cold symptoms and the other two (severe acute respiratory syndrome coronavirus (SARS-CoV) and Middle East respiratory syndrome coronavirus (MERS-CoV)) are zoonotic and producing more severe complications. SARS-CoV and MERS-CoV have caused more than 10,000 cumulative cases in the past two decades, with mortality rates of 34% MERS-CoV and 10% SARS-CoV.

In December 2019, some people that worked at or lived around the Huanan seafood market in Wuhan, Hubei Province, China, have presented pneumonia of unknown cause. Deep sequencing analysis of the respiratory samples indicated a novel coronavirus, which was named firstly 2019 novel coronavirus (2019-nCoV) and lately SARS-CoV-2.

Human-to-human transmission of the SARS-CoV-2 has been confirmed, even in the incubation period without symptoms, and the virus causes severe respiratory illness like those SARS-CoV produced. Although the pneumonia is the principal illness associated, a few patients have developed severe pneumonia, pulmonary edema, acute respiratory distress syndrome, or multiple organ failure and death. Centers of Disease Control and Prevention (CDC) believes that symptoms of SARS-CoV-2 may appear in as few as 2 days or as long as 14 days after exposure, being the most common fever, cough, myalgia and dyspnea. Less common symptoms are sore throat, headache, diarrhea and vomiting. It seems that older males with comorbidities have been more affected.

Diagnosis of SARS-CoV-2 is performed detecting conventional causes of pneumonia early and detected by next-generation sequencing or real-time RT-PCR methods. Several assays that detect the SARS-CoV-2 have been are currently available, such as China CDC (gene targets, ORF1ab and N), Charité – Germany (gene targets, RdRP, E, N) or US CDC (gene targets, three N primers, RdRP).

WHO recommends lower respiratory specimens (sputum, endotracheal aspirate, or bronchoalveolar lavage) for the identification of SARS-CoV-2. However, if the collection is not possible, upper respiratory tract specimens such as a nasopharyngeal aspirate or combined nasopharyngeal and oropharyngeal swabs should be collected. In addition, other clinical specimens as blood, urine and stool may be collected to monitor the presence of the virus.



### 3. Principle of the procedure

VIASURE SARS-CoV-2 Real Time PCR Detection Kit is designed for the diagnosis of SARS-CoV-2 in respiratory samples. The detection is done in one step real time RT format where the reverse transcription and the subsequent amplification of specific target sequence occur in the same reaction well. The isolated RNA target is transcribed generating complementary DNA by reverse transcriptase which is followed by the amplification of a conserved region of *ORF1ab* and *N* genes for SARS-CoV-2 using specific primers and a fluorescent-labeled probe.

VIASURE SARS-CoV-2 Real Time PCR Detection Kit is based on the 5' exonuclease activity of DNA polymerase. During DNA amplification, this enzyme cleaves the probe bounded to the complementary DNA sequence, separating the quencher dye from the reporter. This reaction generates an increase in the fluorescent signal which is proportional to the quantity of target template. This fluorescence can be measured on Real Time PCR platforms.

VIASURE SARS-CoV-2 Real Time PCR Detection Kit contains in each well all the components necessary for real time PCR assay (specific primers/probes, dNTPS, buffer, polymerase and retrotranscriptase) in an stabilized format, as well as an internal control to monitor PCR inhibition. *ORF1ab* gene is amplified and detected in FAM channel, *N* gene is amplified and detected in ROX channel and the internal control (IC) in HEX channel, VIC or JOE channel (depending on the equipment used select the proper detection channel, see Annex 2).

### 4. Reagents provided

VIASURE SARS-CoV-2 Real Time PCR Detection Kit includes the following materials and reagents detailed in Tables 1, 2 and 3. Based on the commercial presentation and the Real Time PCR platform used, the stabilized PCR reaction mix could be placed inside different wells and could be marketed on multiple formats. Table 1 includes materials and reagents to be used with 8-well strips compatible devices (See Annex 1). Table 2 includes materials and reagents to be used with 96-well plate compatible devices (See Annex 1). Table 3 includes materials and reagents for use with Qiagen/Corbett Rotor-Gene® instruments for 4-well strips.

Reagent/Material	Description	Colour	Amount
SARS-CoV-2 8-well strips	A mix of enzymes, primers probes, buffer, dNTPs, stabilizers and Internal control in stabilized format	White	6/12 x 8-well strip
Rehydration Buffer	Solution to reconstitute the stabilized product	Blue	1 vial x 1.8 mL
SARS-CoV-2 Positive Control	Non-infectious synthetic lyophilized cDNA	Red	1 vial
Negative control	Non template control	Violet	1 vial x 1 mL
Water RNase/DNase free	RNase/DNase free water	White	1 vial x 1 mL
Tear-off 8-cap strips	Optical caps for sealing wells during thermal cycling	Transparent	6/12 x 8-cap strip

Table 1. Reagents and materials provided in VIASURE SARS-CoV-2 Real Time PCR Detection Kit with Ref. VS-NCO206L, VS-NCO206H, VS-NCO212L and VS-NCO212H.



Reagent/Material	Description	Color	Amount
SARS-CoV-2 96-well plate	A mix of enzymes, primers probes, buffer, dNTPs, stabilizers and Internal control in stabilized format	White	1 plate
Rehydration Buffer	Solution to reconstitute the stabilized product	Blue	1 vial x 1.8 mL
SARS-CoV-2 Positive Control	Non-infectious synthetic lyophilized cDNA	Red	1 vial
Negative control	Non template control	Violet	1 vial x 1 mL
Water RNase/DNase free	RNase/DNase free water	White	1 vial x 1 mL
Tear-off 8-cap strips	Optical caps for sealing plate during thermal cycling	Transparent	12 x 8-cap strip

Table 2. Reagents and materials provided in VIASURE SARS-CoV-2 Real Time PCR Detection Kit with Ref VS-NCO213L and VS-NCO213H.

Reagent/Material	Description	Colour	Amount
SARS-CoV-2 4-well strips	A mix of enzymes, primers probes, buffer, dNTPs, stabilizers and Internal control in stabilized format	Transparent	9/18 x 4-well strip
Rehydration Buffer	Solution to reconstitute the stabilized product	Blue	1 vial x 1.8 mL
SARS-CoV-2 Positive Control	Non-infectious synthetic lyophilized cDNA	Red	1 vial
Negative control	Non template control	Violet	1 vial x 1 mL
Water RNase/DNase free	RNase/DNase free water	White	1 vial x 1 mL
4-cap strips	Optical caps for sealing wells during thermal cycling	Transparent	9/18 x 4-cap strip

Table 3. Reagents and materials provided in VIASURE SARS-CoV-2 Real Time PCR Detection Kit with Ref. VS-NCO236 and VS-NCO272. For use with Qiagen/Corbett Rotor-Gene® instruments and compatible accessories with strips of 4 tubes 0.1 ml (72-Well Rotor and Locking Ring 72-Well Rotor).

## 5. Reagents and equipment to be supplied by the user

The following list includes the materials that are required for use but not included in the VIASURE SARS-CoV-2 Real Time PCR Detection Kit.

- Real Time PCR instrument (thermocycler).
- RNA extraction kit.
- Centrifuge for 1.5 mL tubes and PCR-well strips or 96-well plate (if available).
- Vortex.
- Micropipettes (0.5-20 µL, 20-200 µL).
- Filter tips.
- Powder-free disposable gloves.
- Loading block (for use with Qiagen/Corbett Rotor-Gene® instruments).

VIASURE SARS-CoV-2 Real Time PCR Detection Kit has been validated on the following equipments: Applied Biosystems 7500 Fast Real-Time PCR System, Applied Biosystems StepOne™ Real-Time PCR System, Bio-Rad CFX96™ Real-Time PCR Detection System, Agilent Technologies AriaMx Real-Time PCR System, DNA-Technology DPrime



Real-time Detection Thermal Cycler, DNA-Technology DTLite Real-Time PCR System, Rotor-Gene® Q (Qiagen), SmartCycler® (Cepheid), Roche Molecular Diagnostics Cobas z480 Analyzer, VIASURE 48 Real Time PCR System and VIASURE 96 Real Time PCR System. When using the Applied Biosystems 7500 Fast with strips it is recommend to place a plate holder to reduce the risk of crushed tube (Ref. PN 4388506).

To check thermocycler compatibility, see Annex 1, to check most common detection channels see Annex 2 and to check optical measurement exposure setting see Annex 3.

## 6. Transport and storage conditions

- The kits can be shipped and stored at 2-40°C until the expiration date which is stated on the label.
- Once the positive control has been re-suspended, store it at -20°C. We recommend to separate it in aliquots to minimize freeze and thaw cycles. Positive control has been validated as still being stable after 6 freeze-thaw cycles.
- Keep components away from sunlight.

## 7. Precautions for users

- The product is indented for use by professional users only, such as laboratory or health professionals and technicians, trained in molecular biological techniques.
- Do not use past expiration date.
- Do not use reagents if the protective pouches are open or broken upon arrival.
- Do not use reagents if desiccant is not present or broken inside reagent pouches.
- Do not remove desiccant from reagent pouches once is open.
- Close protective pouches of reagents promptly with the zip seal after each use (if available, Ref. VS-NCO213L, VS-NCO213H, VS-NCO236 and VS-NCO272). Remove any excess air in the pouches prior to sealing.
- Do not use reagents if the foil has been broken or damaged.
- Do not mix reagents from different envelopes and / or kits and / or lots and / or another supplier.
- Protect reagents against from humidity. Prolonged exposure to humidity may affect product performance.
- For VS-NCO236 and VS-NCO272 (compatible for use with Qiagen/Corbett Rotor-Gene® instruments) use the loading block to pipette reagents and samples into each tube and to help with fitting caps properly and avoid cross contamination.
- Design a unidirectional workflow. It should begin in the Extraction Area and then move to the Amplification and Detection Area. Do not return samples, equipment and reagents to the area in which the previous step was performed.
- Follow Good Laboratory Practices. Wear protective clothing, use disposable gloves, goggles and mask. Do not eat, drink or smoke in the working area. Once you finish the test wash your hands.
- Specimens must be treated as potentially infectious, as well as all the reagents and materials that have been exposed to the samples and they must be handled according to the national safety regulations. Take necessary precautions during the collection, storage, treatment and disposal of samples.





- Regular decontamination of commonly used equipment is recommended, especially micropipettes and work surfaces.
- Consult safety data sheets, upon request.
- Consult each Real Time PCR instrument's reference manual for additional warnings, precautions and procedures.

## 8. Test procedure

### 8.1. RNA extraction

Perform the sample preparation according to the recommendations appearing in the instructions for use of the extraction kit used.

For RNA extraction from respiratory samples you can use your manual or automatic routine optimized system. Also, you can use any commercially available RNA extraction kit and follow the manufacturer's instructions. We have validated the following extraction kits:

- Viasure RNA-DNA Extraction kit (VIASURE), recommended.
- Maxwell® 16 Viral Total Nucleic Acid Purification Kit, using the Maxwell® 16 instrument (Promega).
- Total Nucleic Acid Isolation (TNAI) Kit, using COBAS® AmpliPrep (ROCHE).
- MagDEA Dx SV kit, using the magLEAD® 12gC instrument (Precision System Science Co.).
- MagCore® Viral Nucleic Acid Extraction kit, using the MagCore® HF16 automated Nucleic Acid Extractor System.

### 8.2. Lyophilized positive control

SARS-CoV-2 Positive Control contains high copies of the template, the recommendation is to open and manipulate it in a separate laboratory area away from the other components. Reconstitute the lyophilized SARS-CoV-2 Positive Control (red vial) by adding 100 µL of the supplied Water RNase/DNase free (white vial) and vortex thoroughly.

Once the positive control has been re-suspended, store it at -20°C. We recommend to separate it in aliquots to minimize freeze and thaw cycles.

### 8.3. PCR protocol

Determine and separate the number of required reactions including samples and controls. One positive and negative control must be included in each run for each assay. Peel off protective aluminium seal from plates or strips.

- 1) Reconstitute the number of wells you need.

Add 15 µL of Rehydration Buffer (blue vial) into each well.

- 2) Adding samples and controls.



Add 5 µL of RNA sample, reconstituted SARS-CoV-2 Positive Control (red vial) or Negative Control (violet vial) in different wells and close them with the provided caps. It is recommended to briefly centrifuge the 8-well strips or 96-well plate, or gently tap each strip onto a hard surface to ensure that all the liquids are at the bottom of the tubes (for Qiagen/Corbett Rotor-Gene®).

Load the plate or the strips in the thermocycler.

- 3) Set up the thermocycler (to check compatibility see Annex 1).

Program the thermocycler following the conditions listed below and start the run:

Cycles	Step	Time	Temperature
1	Reverse transcription	15 min	45°C
1	Initial denaturation	2 min	95°C
45	Denaturation	10 seg	95°C
	Annealing/Extension (Data collection*)	50 seg	60°C

Table 4. PCR protocol

Fluorogenic data should be collected during the extension step (\*) through the FAM (*ORF1ab* gene), ROX (*N* gene) and HEX, JOE or VIC (Internal Control (IC)). Depending on the equipment used select the proper detection channel (see Annex 2). In Applied Biosystems 7500 Fast Real-time PCR System, Applied Biosystems StepOne™ Real-Time PCR System and Stratagene Mx3005P™ Real Time PCR System check that passive reference option ROX is none. In the Applied Biosystems 7500 Fast Real-Time PCR System select Ramp Speed Standard in Select New Experiment/Advanced Setup/Experiment Properties.

## 9. Result interpretation

The use of positive and negative controls in each run, validate the reaction by checking the absence of signal in the negative control well and the presence of signal for SARS-CoV-2 in the positive control well. Check Internal Control signal to verify the correct functioning of the amplification mix. The analysis of the samples is done by the software of the used real time PCR equipment itself according to manufacturer's instructions. Using the following table read and analyze the results:



ORF1ab gene (FAM)	N gene (ROX)	Internal control (HEX)	Negative control	Positive control	Interpretation
+	+	+/-	-	+	SARS-CoV-2 Positive
-	-	+	-	+	SARS-CoV-2 Negative
+	-*	+/-	-	+	SARS-CoV-2 Positive*
-**	+	+/-	-	+	SARS-CoV-2 Negative**
+	+	+	+	+	Experiment fail
-	-	-	-	-	Experiment fail

Table 5. Sample interpretation

+: Amplification curve

-: No amplification curve


\* Repeat the extraction and test again, in case of N gene is still negative the interpretation is SARS-CoV-2 Positive.

\*\* Repeat the extraction and test again, if ORF1ab gene is still negative the interpretation is SARS-CoV-2 Negative (Possible infections of other coronavirus).

A sample is considered positive if the Ct value obtained is less than 38 and the internal control shows or not an amplification signal. Sometimes, the detection of internal control is not necessary because a high copy number of target can cause preferential amplification of target-specific nucleic acids.

A sample is considered negative, if the sample shows no amplification signal in the detection system but the internal control is positive. An inhibition of the PCR reaction can be excluded by the amplification of internal control.

Figure 1. Correct run of negative and positive control run on the Bio-Rad CFX96™ Real-Time PCR Detection System.

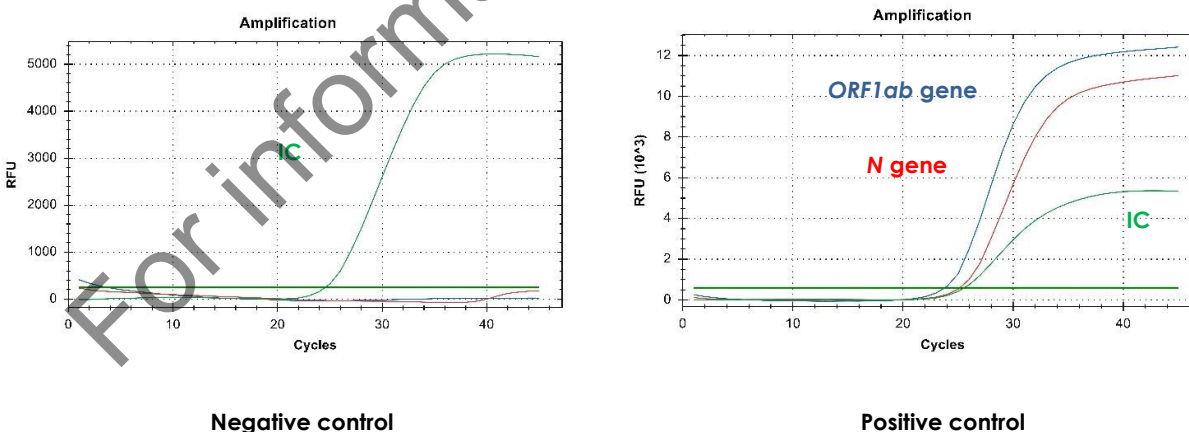

The result is considered invalid if there is signal of amplification in negative control or absence of signal in the positive well. We recommend to repeat the assay again.

In case of absence of internal control signal in sample wells we recommend to repeat the assay diluting the sample 1:10 or to repeat the extraction to check for possible problems of inhibition.





In case of a doubtful interpretation result, it is recommended to verify the correct performance of each of the steps and review the parameters and the sigmoid shape of the curve. If the situation is not solved, it is recommended to repeat the assay, preferably in duplicate. The results of the test should be evaluated by a health care professional in the context of medical history, clinical symptoms and other diagnostic tests.

## 10. Limitations of the test

- The results of the test should be evaluated by a health care professional in the context of medical history, clinical symptoms and other diagnostic tests.
- Although this assay can be used with other types of samples it has been validated only with RNA extracted from respiratory samples (nasopharyngeal swab and oropharyngeal swab).
- The quality of the test depends on the quality of the sample; proper extracted nucleic acid from clinical samples must be extracted. Unsuitable collection, storage and/or transport of specimens may give false negative results.
- Extremely low levels of target below the limit of detection might be detected, but results may not be reproducible.
- There is a possibility of false positive results due to cross-contamination by SARS-CoV-2, either samples containing high concentrations of target RNA or contamination due to PCR products from previous reactions.

## 11. Quality control

VIASURE SARS-CoV-2 Real Time PCR Detection Kit contains a positive and a negative control that must be included in each run to correctly interpret the results. Also, the internal control (IC) in each well confirms the correct performance of the technique.

## 12. Performance characteristics

### 12.1. Clinical sensitivity and specificity

The clinical performance of VIASURE SARS-CoV-2 Real Time PCR Detection Kit was tested using 100 respiratory specimens (nasopharyngeal swab) from symptomatic patients with suspicion of COVID-19. These results were compared with those obtained with a molecular detection method by the Spanish National Reference Center (Institute of Health Carlos III (ISCIII)). The results were as follows:

VIASURE SARS-CoV-2 Real Time PCR Detection Kit	Molecular detection method			Total
		+	-	
+	2	0	2	
-	0	98	98	
Total	2	98	100	

Table 6. Comparative results for SARS-CoV-2.



Besides, another clinical evaluation of VIASURE SARS-CoV-2 Real Time PCR Detection Kit was conducted with 34 contrived oropharyngeal swabs collected in viral transport media (VTM). 10 negative oropharyngeal swabs were spiked with RNA from Human 2019-nCoV strain BetaCoV/Germany/BavPat1/2020 p.1, and another 12 negative specimens were spiked with a known concentration of each cDNA control templates and were tested blindly. 33/34 spiked samples were detected correctly.

The results show a high sensitivity and specificity to detect SARS-CoV-2 using VIASURE SARS-CoV-2 Real Time PCR Detection Kit.

### 12.2. Analytical sensitivity

VIASURE SARS-CoV-2 Real Time PCR Detection Kit has a detection limit of  $\geq 10$  RNA copies per reaction for *ORF1ab* and *N* genes (Figures 2 and 3).

Figure 2. Dilution series of *ORF1ab* gene ( $10^7$ - $10^1$  copies/rxn) template run on the Bio-Rad CFX96™ Real-Time PCR Detection System (FAM channel).


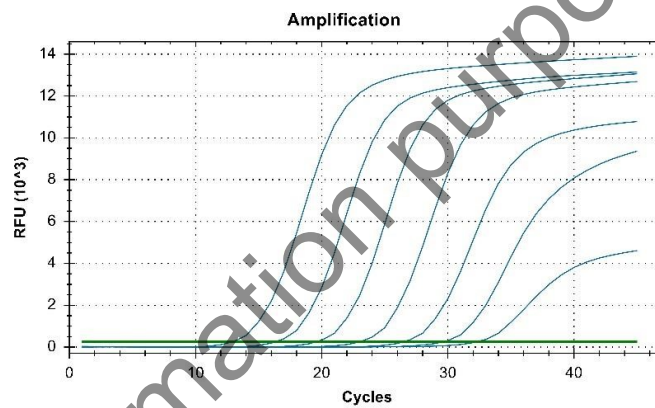


Figure 3. Dilution series of *N* gene ( $10^7$ - $10^1$  copies/rxn) template run on the Bio-Rad CFX96™ Real-Time PCR Detection System (ROX channel).

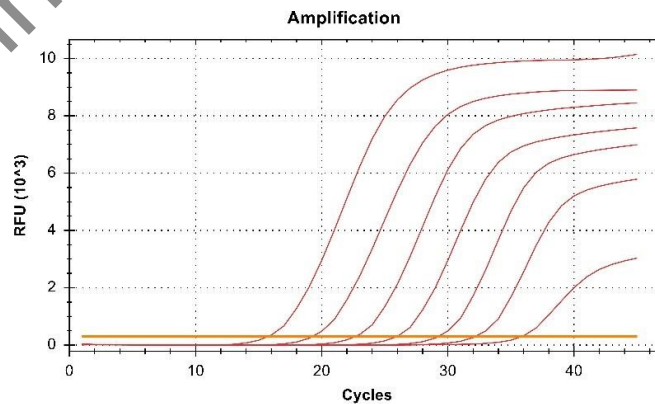

### 12.3. Analytical specificity

The specificity of the SARS-CoV-2 assay was confirmed by testing a panel consisting of different microorganisms representing the most common respiratory pathogens. No cross-reactivity was detected between any of the following microorganisms tested.

Cross-reactivity testing					
<i>Bordetella pertussis</i>	-	<i>Streptococcus pneumoniae</i> Z022	-	Influenza A/Anhui/1/2013 (H7N9) virus	-
<i>Bordetella parapertussis</i>	-	<i>Staphylococcus aureus</i> subsp. <i>aureus</i>	-	Influenza B/Brisbane/60/2008 virus	-
<i>Bordetella holmesii</i>	-	<i>Moraxella catarrhalis</i>	-	Influenza B/Florida/04/06 virus	-
<i>Bordetella bronchiseptica</i>	-	<i>Mycobacterium tuberculosis</i> not rifampin resistant	-	Influenza B/Phuket/3073/2013 virus	-
<i>Haemophilus influenzae</i> MinnA	-	<i>Pneumocystis jirovecii</i>	-	Human parainfluenza 1, 2, 3 and 4 viruses	-
<i>Chlamydia caviae</i>	-	Influenza A/New Caledonia/20/99(H1N1) virus	-	Human metapneumovirus A and B	-
<i>Chlamydia psittaci</i> genotypes A and C	-	Influenza A/California/7/2009(H1N1) virus	-	Human rhinovirus type C	-
<i>Chlamydophila pneumoniae</i> CM-1	-	Influenza A/Michigan/45/2015 (H1N1)pdm09 virus	-	Human Adenovirus Types 1-5, 8, 15, 31, 40 and 41	-
<i>Legionella bozemanii</i>	-	Influenza A/Singapore/GP1908/2015 (H1N1)pdm09 virus	-	Human Bocavirus	-
<i>Legionella micdadei</i>	-	Influenza A/Perth/16/2009(H3N2) virus	-	Respiratory Syncytial virus (RSV) A and B	-
<i>Legionella dumoffii</i>	-	Influenza A/Thüringen/5/2017 (H3N2) virus	-	Human coronavirus 229E, OC43, NL63 and HKU1	-
<i>Legionella pneumophila</i>	-	Influenza A/Switzerland/9715293/2013 (H3N2) virus	-	MERS Coronavirus	-
<i>Legionella longbeache</i>	-	Influenza A/Hong Kong/4801/2014(H3N2) virus	-	SARS Coronavirus Strain Frankfurt 1	-
<i>Mycoplasma pneumoniae</i>	-	Influenza A/DE-SH/Reiherente/AR8444/2016 (H5N8) virus	-		-

Table 7. Reference pathogenic microorganisms used in this study

### 12.4. Analytical reactivity

The reactivity of VIASURE SARS-CoV-2 Real Time PCR Detection Kit was evaluated against RNA from Human 2019-nCoV strain BetaCoV/Germany/BavPat1/2020 p.1 showing positive results.



ANNEX 1

**COMPATIBILITY WITH THE MOST COMMON REAL TIME PCR EQUIPMENT**

Low profile strips can be used in all PCR thermocyclers equipped with a low profile block, like the systems listed in table A.1. High profile strips can be used in all PCR thermocyclers equipped with a high or regular profile block, like the systems listed in table A.2. If you do not find your thermocycler in the list below, please contact with your supplier.

Table A.1 LOW PROFILE BLOCK THERMOCYCLERS	
Manufacturer	Model
Agilent Technologies	AriaMx/AriaDx Real-Time PCR System
Applied Biosystems	7500 Fast Real-Time PCR System <sup>(1)</sup>
Applied Biosystems	7500 Fast Dx Real-Time PCR System <sup>(1)</sup>
Applied Biosystems	QuantStudio™ 12K Flex 96-well Fast
Applied Biosystems	QuantStudio™ 6 Flex 96-well Fast
Applied Biosystems	QuantStudio™ 7 Flex 96-well Fast
Applied Biosystems	QuantStudio™ 3 Fast Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	QuantStudio™ 5 Fast Real-Time PCR System
Applied Biosystems	StepOne Plus™ Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	StepOne™ Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	ViiA™ 7 Fast Real-Time PCR System
BIONEER	Exicycler™ 96
Bio-Rad	CFX96™ / CFX96™ IVD Real-Time PCR Detection System
Bio-Rad	Mini Opticon™ Real-Time PCR Detection System <sup>(4)</sup>
Cepheid	SmartCycler® <sup>(3)</sup>
Qiagen	Rotor-Gene® Q <sup>(3)</sup>
Roche	LightCycler® 480 Real-Time PCR System <sup>(4)</sup>
Roche	LightCycler® 96 Real-Time PCR System <sup>(4)</sup>
Roche	Cobas z480 Analyzer <sup>(4)</sup>

Table A.2 HIGH PROFILE BLOCK THERMOCYCLERS	
Manufacturer	Model
Abbott	Abbott m2000 RealTime System
Applied Biosystems	7300 Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	7500 Real-Time PCR System
Applied Biosystems	7900 HT Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	ABI PRISM 7000 <sup>(4)</sup>
Applied Biosystems	ABI PRISM 7700 <sup>(5)</sup>
Applied Biosystems	QuantStudio™ 12K Flex 96-well
Applied Biosystems	QuantStudio™ 6 Flex 96-well
Applied Biosystems	QuantStudio™ 7 Flex 96-well
Applied Biosystems	QuantStudio™ 3 Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	QuantStudio™ 5 Real-Time PCR System
Applied Biosystems	ViiA™ 7 Real-Time PCR System
Analytik Jena Biometra	TOptical
Analytik Jena Biometra	qTOWER 2.0
BIONEER	Exicycler™ 96
Bio-Rad	CFX96™ Deep Well / CFX96™ Deep Well IVD Real-Time PCR Detection System
Bio-Rad	iCycler iQ™ Real-Time PCR Detection System
Bio-Rad	iCycler iQ™5 Real-Time PCR Detection System
Bio-Rad	MyiQ™ Real-Time PCR Detection System <sup>(6)</sup>
Bio-Rad	MyiQ™2 Real-Time PCR Detection System <sup>(6)</sup>
Cepheid	SmartCycler® <sup>(3)</sup>
DNA-Technology	DTprime Real-time Detection Thermal Cycler <sup>(2)</sup>
DNA-Technology	DTlite Real-Time PCR System <sup>(2)</sup>
Eppendorf	Mastercycler™ep realplex
Qiagen	Rotor-Gene® Q <sup>(3)</sup>
Stratagene / Agilent Technologies	Mx3000P™ Real Time PCR System
Stratagene / Agilent Technologies	Mx3005P™ Real Time PCR System

(1) Select Ramp Speed "Standard".  
 (2) See Annex 3 to check optical measurement exposure setting.  
 (3) The product should be reconstituted following the appropriate procedure (see Test Procedure) and transferred into the specific Rotor-Gene® Q or SmartCycler® tubes.  
 (4) Shell Frame grid plate which fits in these Roche qPCR System is necessary.  
 (5) No detection in Cy5 channel.  
 (6) Detection in FAM and HEX channels only.

Table A1/A2. Compatible low and high profile Real Time PCR systems.



ANNEX 2

**DETECTION CHANNELS FOR THE MOST COMMON REAL TIME PCR EQUIPMENT**

The fluorescence detection channels for some of most common Real Time PCR Thermocyclers are specified in Table A3.

REAL-TIME PCR THERMOCYCLER	VIASURE CHANNEL	DETECTION CHANNEL	OBSERVATIONS
Bio-Rad CFX96™	FAM	FAM	Some wells may have abnormally drifting RFU values during the initial few cycles of a run showing a non-sigmoidal ascendant line. If you see this effect, in the Settings menu, select the option Apply Fluorescence Drift Correction for Baseline Settings to correct it.
	HEX	HEX	
	ROX	ROX	
	Cy5	Cy5	
ABI 7500 Applied Biosystems	FAM	FAM	Passive reference option for ROX must be none. Some wells may have abnormally drifting RFU values during the initial few cycles of a run showing a non-sigmoidal ascendant line. If you see this effect, please modify the baseline: Select the Start Cycle and End Cycle values so that the baseline ends before significant fluorescence is detected.
	HEX	VIC	
	ROX	ROX	
	Cy5	Cy5	
Roche Lightcycler®480II	FAM	465/510	Colour Compensation is required
	HEX	533/580	
	ROX	533/610	
	Cy5	618/660	
Smartcycler® Cepheid	FAM	Channel 1	
	HEX	Channel 2	
	ROX	Channel 3	
	Cy5	Channel 4	
Abbott m2000rt	FAM	FAM	
	HEX	VIC	
	ROX	ROX	
	Cy5	Cy5	
Mx3000P™ Mx 3005P™ Stratagene	FAM	FAM	Passive reference option for ROX must be none
	HEX	VIC	
	ROX	ROX	
	Cy5	Cy5	
AriaMx Agilent	FAM	FAM	
	HEX	HEX	
	ROX	ROX	
	Cy5	Cy5	
Rotor-Gene®Q Qiagen	FAM	Green	In the Channel Setup, click on the "Gain Optimisation" button and then go to "Optimise Acquiring". The fluorescence Target Sample Range has to be between 5 and 10 FI for each channel. Also select the option "Perform Optimisation Before 1st Acquisition".
	HEX	Yellow	
	ROX	Orange	
	Cy5	Red	
Mic Real Time PCR Cycler bms	FAM	Green	In the "Run Profile" menu, introduce the correct parameters for "Temperature Control" (Standard TAQ (v3)), Volume (20 ul) and the appropriate thermal profile. In the "Cycling" window, select the "Acquire on" option for all the channels by clicking on them. Use the default "Gain" values for each channel (Green = 3, Yellow = 10, Orange = 10, Red = 10)
	HEX	Yellow	
	ROX	Orange	
	Cy5	Red	
Exicycler™ 96 BIONEER	FAM	FAM	
	HEX	JOE	
	ROX	ROX	
	Cy5	Cy5	

Table A3: Detection fluorescence channels of different Real Time PCR systems.



## ANNEX 3

**OPTICAL MEASUREMENT EXPOSURE SETTING**

Optical measurement parameters of some thermocyclers must be adjusted to be suitable for operation with "VIASURE Real Time PCR Detection Kits". This assay has been validated with the following set exposition values:

- DTprime Real-time Detection Thermal Cycler (DNA-Technology): FAM channel -500\*, HEX channel – 1000, ROX channel – 1000 and Cy5 channel - 1000.
- DTlite Real-Time PCR System (DNA-Technology): FAM channel - 500, HEX channel - 500, ROX channel – 500 and Cy5 channel - 500.

\*If the result in channel FAM is not as expected, there are no amplifications or high background noise is observed, please lower the exposure values indicated above to 150.

For information purposes only





## ESPAÑOL

### 1. Uso previsto

VIASURE SARS-CoV-2 Real Time PCR Detection Kit está diseñado para la identificación y diferenciación específica del 2019 Nuevo Coronavirus (SARS-CoV-2) en muestras respiratorias procedentes de pacientes con signos y síntomas de COVID-19. El uso previsto del test es facilitar el diagnóstico de infección producida por SARS-CoV-2 en combinación con factores de riesgos clínicos y epidemiológicos. El RNA es extraído a partir de los especímenes respiratorios, posteriormente el DNA complementario es sintetizado en un solo paso y amplificado mediante PCR a tiempo real. La detección se lleva a cabo utilizando oligonucleótidos específicos y una sonda marcada con una molécula fluorescente y otra apantalladora (*quencher*) para detectar SARS-CoV-2.

### 2. Introducción y explicación

Los coronavirus son virus envueltos de RNA de cadena positiva no segmentados que pertenecen a la familia *Coronaviridae*. Se conocen seis especies de coronavirus que causan enfermedades humanas: cuatro virus (229E, OC43, NL63 y HKU1) que causan síntomas de resfriado común, y otros dos (coronavirus asociado a síndrome respiratorio agudo grave- severe acute respiratory syndrome coronavirus, SARS-CoV-, y el coronavirus causante del síndrome respiratorio de Oriente Medio - Middle East respiratory syndrome coronavirus, MERS-CoV-) que son zoonóticos y producen complicaciones más severas. SARS-CoV y MERS-CoV han causado más de 10.000 casos acumulados en las últimas dos décadas, con unas tasas de mortalidad del 34% para MERS-CoV y 10% para SARS-CoV.

En diciembre de 2019, algunas personas que trabajaban o vivían alrededor del mercado de mariscos de Huanan en Wuhan, provincia de Hubei, China, presentaron neumonía de causa desconocida. El análisis de secuenciación masiva de las muestras respiratorias mostró un nuevo coronavirus, que fue llamado inicialmente como 2019 nuevo coronavirus (2019-nCoV) y posteriormente como SARS-CoV-2.

Se ha confirmado la transmisión de persona a persona del SARS-CoV-2, incluso en el período de incubación en asintomáticos, y el virus causa enfermedad respiratoria severa como la producida por el SARS-CoV. Aunque la neumonía es la principal enfermedad asociada, algunos pacientes han desarrollado neumonía severa, edema pulmonar, síndrome de dificultad respiratoria aguda o fallo multiorgánico y muerte. Los Centros para el Control y la Prevención de Enfermedades (Centers of Disease Control and Prevention, CDC) cree que los síntomas del SARS-CoV-2 pueden aparecer en tan solo dos días o hasta 14 tras la exposición, siendo los más comunes fiebre, tos, mialgia y disnea. Aquellos síntomas menos comunes son dolor de garganta, dolor de cabeza, diarrea y vómitos. Parece que los hombres mayores con comorbilidades se han visto más afectados.

El diagnóstico del SARS-CoV-2 se realiza detectando las causas convencionales de la neumonía temprana y por secuenciación masiva o métodos de RT-PCR a tiempo real. Actualmente se encuentran disponibles varios ensayos que detectan el SARS-CoV-2, como China CDC (genes objetivos, ORF1ab and N), Charité – Alemania (genes objetivos, RdRP, E, N) o Estados Unidos CDC (genes objetivos, three N primers, RdRP).

WHO recomienda muestras de las vías respiratorias inferiores (esputos, aspirados endotraqueales o lavados broncoalveolares) para la identificación del SARS-CoV-2. Sin embargo, si la recolección no es posible, se deben



tomar las muestras del tracto respiratorio superior como aspirados nasofaríngeos o hisopos nasofaríngeos y orofaríngeos combinados. Además, se pueden recolectar otras muestras clínicas como sangre, orina y heces para controlar la presencia del virus.

### 3. Procedimiento

VIASURE SARS-CoV-2 Real Time PCR Detection Kit está diseñado para el diagnóstico de SARS-CoV-2 en muestras respiratorias. La detección se realiza a través de la retrotranscripción y posterior amplificación a tiempo real de la secuencia diana, produciéndose ambas reacciones en el mismo pocillo. Tras el aislamiento del RNA, se sintetiza el DNA complementario a la secuencia diana gracias a la retrotranscriptasa o transcriptasa inversa. Posteriormente la identificación de SARS-CoV-2 se lleva a cabo mediante la reacción en cadena de la polimerasa utilizando oligonucleótidos específicos y una sonda marcada con fluorescencia que hibridan con una región diana conservada de los genes *ORF1ab* y *N*.

VIASURE SARS-CoV-2 Real Time PCR Detection Kit aprovecha la actividad 5' exonucleasa de la DNA-polimerasa. Durante la amplificación del DNA, esta enzima hidroliza la sonda unida a la secuencia de DNA complementaria, separando el fluoróforo del *quencher*. Esta reacción genera un aumento en la señal fluorescente proporcional a la cantidad de RNA diana. Esta fluorescencia se puede monitorizar en equipos de PCR a tiempo real.

VIASURE SARS-CoV-2 Real Time PCR Detection Kit contiene en cada pocillo todos los componentes necesarios para llevar a cabo la PCR a tiempo real (cebadores/sondas específicos, dNTPS, tampón, polimerasa, retrotranscriptasa) en formato estabilizado, así como, un control interno para descartar la inhibición de la actividad polimerasa. Tras la reacción de amplificación, el gen *ORF1ab* se detecta en el canal FAM, el gen *N* se detecta en el canal ROX y el control interno (CI) se detecta en el canal HEX, VIC o JOE (seleccionar el canal de detección según el equipo utilizado, ver Anexo 2).

### 4. Reactivos suministrados

VIASURE SARS-CoV-2 Real Time PCR Detection Kit incluye los siguientes materiales y reactivos detallados en las Tablas 1, 2 y 3. Basado en la presentación comercial y la plataforma de PCR en tiempo real utilizada, la mezcla de reacción de PCR estabilizada se puede encontrar en diferentes tubos o pocillos y por tanto comercializar en múltiples formatos. La Tabla 1 incluye materiales y reactivos para usar con dispositivos compatibles para tiras de 8 pocillos (Ver Anexo 1). La Tabla 2 incluye materiales y reactivos para usar con dispositivos compatibles para placas de 96 pocillos (Ver Anexo 1). La Tabla 3 incluye materiales y reactivos para usar con los instrumentos Qiagen / Corbett Rotor-Gene® para tiras de 4 pocillos.



Reactivo/Material	Descripción	Color	Cantidad
SARS-CoV-2 8-well strips	Una mezcla de enzimas, cebadores-sondas, tampón, dNTPs, estabilizadores y Control interno en formato estabilizado	Blanco	6/12 tiras de 8 pocillos
Rehydration Buffer	Solución para la reconstitución del producto estabilizado	Azul	1 vial x 1.8 mL
SARS-CoV-2 Positive Control	cDNA sintético liofilizado no infeccioso	Rojo	1 vial
Negative control	Control negativo	Morado	1 vial x 1 mL
Water RNase/DNase free	Agua libre de RNAsa/DNAsa	Blanco	1 vial x 1 mL
Tear-off 8-cap strips	Tapones ópticos para sellar los pocillos durante el ciclo térmico	Transparente	6/12 tiras de 8 tapones

Tabla 1. Reactivos y materiales proporcionados en VIASURE SARS-CoV-2 Real Time PCR Detection Kit con Ref. VS-NCO206L, VS-NCO206H, VS-NCO212L y VS-NCO212H.

Reactivo/Material	Descripción	Color	Cantidad
SARS-CoV-2 96-well plate	Una mezcla de enzimas, cebadores-sondas, tampón, dNTPs, estabilizadores y Control interno en formato estabilizado	Blanco	1 placa
Rehydration Buffer	Solución para la reconstitución del producto estabilizado	Azul	1 vial x 1.8 mL
SARS-CoV-2 Positive Control	cDNA sintético liofilizado no infeccioso	Rojo	1 vial
Negative control	Control negativo	Morado	1 vial x 1 mL
Water RNase/DNase free	Agua libre de RNAsa/DNAsa	Blanco	1 vial x 1 mL
Tear-off 8-cap strips	Tapones ópticos para sellar los pocillos durante el ciclo térmico	Transparente	12 tiras de 8 tapones

Tabla 2. Reactivos y materiales proporcionados en VIASURE SARS-CoV-2 Real Time PCR Detection Kit con Ref. VS-NCO213L y VS-NCO213H.

Reactivo/Material	Descripción	Color	Cantidad
SARS-CoV-2 4-well strips	Una mezcla de enzimas, cebadores-sondas, tampón, dNTPs, estabilizadores y Control interno en formato estabilizado	Transparente	9/18 tiras de 4 pocillos
Rehydration Buffer	Solución para la reconstitución del producto estabilizado	Azul	1 vial x 1.8 mL
SARS-CoV-2 Positive Control	cDNA sintético liofilizado no infeccioso	Rojo	1 vial
Negative control	Control negativo	Morado	1 vial x 1 mL
Water RNase/DNase free	Agua libre de RNAsa/DNAsa	Blanco	1 vial x 1 mL
4-cap strips	Tapones ópticos para sellar los pocillos durante el ciclo térmico	Transparente	9/18 tiras de 4 tapones

Tabla 3. Reactivos y materiales proporcionados en VIASURE SARS-CoV-2 Real Time PCR Detection Kit con Ref. VS-NCO236 y VS-NCO272. Para usar con instrumentos Qiagen / Corbett Rotor-Gene® y accesorios compatibles con tiras de 4 tubos 0.1 ml (72-Well Rotor y Locking Ring 72-Well Rotor).



## 5. Material requerido y no suministrado

La siguiente lista incluye los materiales que se requieren para el uso pero que no se incluyen en VIASURE SARS-CoV-2 Real Time PCR Detection Kit.

- Equipo de PCR a tiempo real (termociclador).
- Kit de extracción de RNA.
- Centrífuga para tubos de 1.5 mL y para tiras de tubos de PCR o placas de 96 pocillos (si está disponible).
- Vórtex.
- Micropipetas (0.5-20 µL, 20-200 µL).
- Puntas con filtro.
- Guantes desechables sin polvo.
- Loading block (para usar con instrumentos Qiagen/Corbett Rotor-Gene®).

VIASURE SARS-CoV-2 Real Time PCR Detection Kit ha sido validado en los siguientes equipos: Applied Biosystems 7500 Fast Real-Time PCR System, Applied Biosystems StepOne™ Real-Time PCR System, Bio-Rad CFX96™ Real-Time PCR Detection System, Agilent Technologies AriaMx Real-Time PCR System, DNA-Technology DTprime Real-time Detection Thermal Cycler, DNA-Technology DTLite Real-Time PCR System, Rotor-Gene® Q (Qiagen), SmartCycler® (Cepheid), Roche Molecular Diagnostics Cobas z480 Analyzer, VIASURE 48 Real Time PCR System y VIASURE 96 Real Time PCR System. Cuando se utiliza el equipo Applied Biosystems 7500 Fast con tiras, se recomienda colocar el soporte adecuado para reducir el riesgo de aplastar el tubo (Ref. PN 4388506).

Para verificar la compatibilidad de los termocicladores, consulte el Anexo 1, para verificar los canales de detección más comunes, consulte el Anexo 2 y para verificar la configuración de la exposición de medición óptica, ver Anexo 3.

## 6. Condiciones de transporte y almacenamiento

- El transporte y almacenaje de los kits puede realizarse de 2-40°C hasta la fecha de caducidad indicada en la etiqueta.
- Almacenar el control positivo a -20°C tras su re-suspensión. Se recomienda separar en alícuotas para minimizar los ciclos de congelación y descongelación. Se ha validado la estabilidad del control positivo tras 6 ciclos de congelación y descongelación.
- Proteger los componentes de la luz.

## 7. Precauciones para el usuario

- El producto está destinado para uso exclusivo de usuarios profesionales, como profesionales o técnicos de laboratorio y sanitarios, entrenados en técnicas de biología molecular.
- No se recomienda usar el kit después de la fecha de caducidad.
- No utilizar los reactivos si los sobres o las bolsas que protegen los tubos están abiertos o dañados en el momento que se reciben.



- No utilizar los tubos de reacción si el material desecante que se incluye en cada sobre de aluminio no está o está dañado.
- No retirar el material desecante de los sobres de aluminio que contienen los tubos de reacción una vez abiertos.
- Cerrar los sobres de aluminio que protegen los tubos de reacción con el cierre zip inmediatamente después de cada uso (si está disponible, Ref. VS-NCO213L, VS-NCO213H, VS-NCO236 y VS-NCO272). Antes de cerrar los sobres eliminar cualquier exceso de aire.
- No utilizar los tubos de reactivos si el aluminio protector está roto o dañado.
- No mezclar reactivos de diferentes sobres y/o kits y/o lotes y/u otro proveedor.
- Proteger los reactivos de la humedad. Una exposición prolongada a la humedad puede afectar al rendimiento del producto.
- Para VS-NCO236 y VS-NCO272 (compatible con instrumentos Qiagen/Corbett Rotor-Gene®) utilice el loading block para pipetear reactivos y muestras en cada tubo y para ayudar en el ajuste correcto de las tapas así como para evitar la contaminación.
- Diseñar un flujo de trabajo unidireccional. Se debe comenzar en el área de extracción y después pasar al área de amplificación y de detección. No poner en contacto las muestras, equipos y reactivos utilizados en un área con la zona en la que se realizó el paso anterior.
- Seguir las Buenas Prácticas de Laboratorio. Use ropa protectora, guantes de uso desechables, gafas y mascarilla. No comer, beber o fumar en el área de trabajo. Una vez terminada la prueba, lavarse las manos.
- Las muestras deben ser tratadas como potencialmente infecciosas así como los reactivos que han estado en contacto con las muestras y deben ser gestionadas según la legislación sobre residuos sanitarios nacional. Tome las precauciones necesarias durante la recogida, almacenamiento, tratamiento y eliminación de muestras.
- Se recomienda la descontaminación periódica de los equipos usados habitualmente, especialmente micropipetas, y de las superficies de trabajo.
- Consulte las hojas de seguridad, previa solicitud.
- Consulte el manual de cada equipo de PCR a tiempo real para advertencias adicionales, precauciones y procedimientos.

## 8. Procedimiento del test

### 8.1. Extracción de RNA

Realizar la preparación de la muestra de acuerdo con las recomendaciones que aparecen en las instrucciones de uso del kit de extracción utilizado.

Para la extracción de RNA a partir de muestras respiratorias puede utilizar su sistema optimizado de rutina manual o automático. Además, se puede usar cualquier kit de extracción de RNA disponible en el mercado y seguir las instrucciones de uso del fabricante. Los siguientes kits de extracción han sido validados:

- Viasure RNA-DNA Extraction kit (VIASURE), recomendado.



- Maxwell® 16 Viral Total Nucleic Acid Purification Kit, utilizando el sistema de extracción automatizado Maxwell® 16 instrument (Promega).
- Total Nucleic Acid Isolation (TNAI) Kit, utilizando el sistema de extracción automatizado COBAS® AmpliPrep (ROCHE).
- MagDEA Dx SV kit, empleando el instrumento magLEAD® 12gC (Precision System Science Co.).
- MagCore® Viral Nucleic Acid Extraction kit, empleando el instrumento MagCore® HF16 automated Nucleic Acid Extractor System.

## 8.2. Control positivo liofilizado

El vial de SARS-CoV-2 Positive Control contiene una gran cantidad de copias molde por lo que se recomienda abrirlo y manipularlo en una zona del laboratorio separada del resto de los componentes. Reconstituir SARS-CoV-2 Positive Control liofilizado (vial rojo) añadiendo 100 µL de Agua libre de RNAsa/DNAsa (vial blanco) suministrada y mezclar bien con la ayuda del vórtex.

Almacenar el control positivo a -20°C tras su re-suspensión. Se recomienda separar en alícuotas para minimizar los ciclos de congelación y descongelación.

## 8.3. Protocolo PCR

Determinar y separar el número de reacciones necesarias incluyendo las muestras y los controles. En cada serie de muestras para cada uno de los ensayos a analizar se deben incluir un control positivo y uno negativo. Retirar el aluminio protector de las placas o tiras.

- 1) Reconstituir el número de pocillos que sean necesarios.

Añadir 15 µL del tampón de rehidratación (vial azul) en cada pocillo.

- 2) Añadir muestras y controles.

Añadir 5 µL de RNA extraído de cada muestra, de SARS-CoV-2 Positive Control reconstituido (vial rojo) o Negative Control (vial morado) y cerrar los pocillos con los tapones suministrados. Se recomienda centrifugar brevemente las tiras de 8 pocillos o las placas de 96 pocillos, o golpear suavemente cada tira sobre una superficie dura para asegurarse de que todos los líquidos queden en el fondo de los tubos (para los kits compatible con Qiagen/Corbett Rotor-Gene®).

Colocar la placa o las tiras en el termociclador.

- 3) Configurar el termociclador (para verificar la compatibilidad, consulte el Anexo 1).

Programar el termociclador siguiendo las condiciones descritas en la siguiente tabla e iniciar el programa:





Ciclos	Etapa	Tiempo	Temperatura
1	Retrotranscripción	15 min	45°C
1	Desnaturalización inicial	2 min	95°C
45	Desnaturalización	10 seg	95°C
	Hibridación/Elongación (Recogida de datos*)	50 seg	60°C

Tabla 4. Protocolo PCR

Los datos de fluorescencia deben recogerse durante la etapa de elongación (\*) a través de los canales FAM (gen *ORF1ab*), ROX (gen *N*) y HEX, JOE o VIC (Control Interno). En los termocicladores Applied Biosystems 7500 Fast Real-Time PCR System, Applied Biosystems StepOne™ Real-Time PCR System y Stratagene Mx3005PT™ Real Time PCR System comprobar que la opción del control pasivo ROX está desactivada. En el termociclador Applied Biosystems 7500 Fast Real-Time PCR System seleccionar Ramp Speed Standard en el menú Select New Experiment/Advanced Setup/Experiment Properties.

## 9. Interpretación de resultados

El uso de los controles positivo y negativo junto con cada serie de muestras a analizar, valida la reacción comprobando la ausencia de señal en el pocillo del control negativo y la presencia de una señal en el pocillo de control positivo para el SARS-CoV-2. Comprobar la emisión de la señal del control interno para verificar el correcto funcionamiento de la mezcla de amplificación. El análisis de las muestras se realiza con el software propio del equipo de PCR a tiempo real de acuerdo con las instrucciones de uso del fabricante. Con ayuda de la siguiente tabla, leer y analizar los resultados:

Gen <i>ORF1ab</i> (FAM)	Gen <i>N</i> (ROX)	Control interno (HEX)	Control Negativo	Control Positivo	Interpretación
+	+	+/-	-	+	SARS-CoV-2 Positivo
-	-	+	-	+	SARS-CoV-2 Negativo
+	-*	+/-	-	+	SARS-CoV-2 Positivo*
-**	+	+/-	-	+	SARS-CoV-2 Negativo**
+	+	+	+	+	Inválido
	-	-	-	-	Inválido

Tabla 5. Interpretación

+ : curva de amplificación

- : sin curva de amplificación

\* Repetir la extracción y el ensayo de nuevo, en caso de que gen *N* continúe siendo negativo la interpretación será SARS-CoV-2 Positivo.

\*\* Repetir la extracción y el ensayo de nuevo, si el gen *ORF1ab* continúa siendo negativo la interpretación será SARS-CoV-2 Negativo (Posibles infecciones de otros coronavirus).


Una muestra se considera positiva, si el valor Ct obtenido es menor de 38 y el control interno muestra o no una gráfica de amplificación. En ocasiones, la detección del control interno no es necesaria, ya que la presencia de



un alto número inicial de copias del ácido nucleico diana puede causar una amplificación preferencial de esta última.

Una muestra se considera negativa, si no se detecta una curva de amplificación por encima del valor umbral, y el control interno si la presenta. La inhibición de la reacción de PCR puede ser excluida por la amplificación del control interno.

Figura 1. Ejemplo de gráficas de amplificación del control negativo y positivo. Experimento realizado en el equipo Bio-Rad CFX96™ Real-Time PCR Detection System.

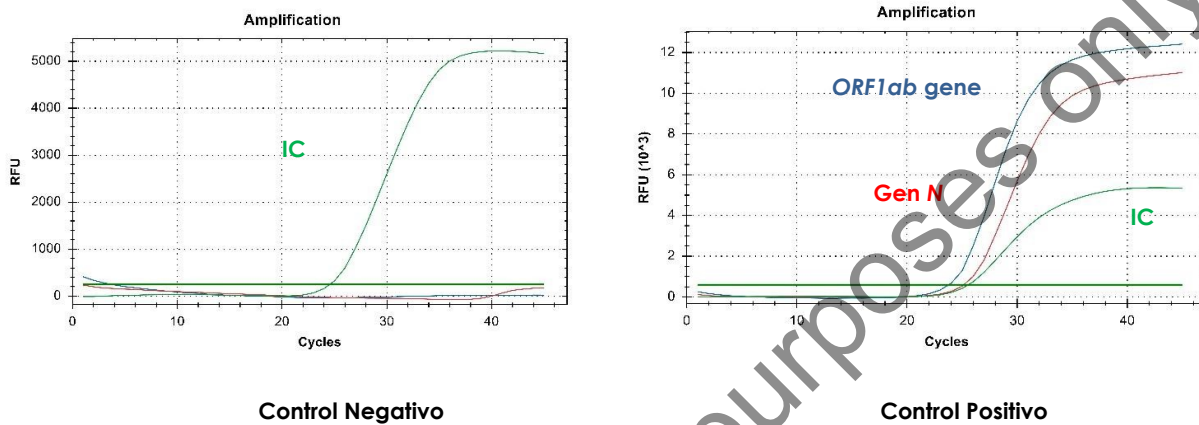

El resultado se considera inválido si se observa una gráfica de amplificación en el control negativo o ausencia de señal en el pocillo del control positivo. En ese caso, se recomienda repetir el ensayo.

En caso de ausencia de la señal de control interno en los pocillos de muestra, se recomienda repetir el ensayo diluyendo la muestra 1:10 o repetir la extracción para descartar posibles problemas de inhibición.

En el caso de obtener un resultado de dudosa interpretación, se recomienda verificar la correcta realización de cada uno de los pasos y revisar los parámetros y la forma sigmoidea de la curva. Si la situación no se resuelve, se recomienda repetir el ensayo, preferiblemente por duplicado. El resultado de la prueba debe ser evaluado en el contexto del historial médico, los síntomas clínicos y otras pruebas de diagnóstico por un profesional de la salud.

## 10. Limitaciones del test

- El resultado de la prueba debe ser evaluado en el contexto del historial médico, los síntomas clínicos y otras pruebas de diagnóstico por un profesional de la salud.
- Este ensayo se podría utilizar con diferentes tipos de muestras, aunque sólo ha sido validado con RNA extraído de muestras respiratorias (frotis nasofaríngeo y orofaríngeo).
- El correcto funcionamiento de la prueba depende de la calidad de la muestra; el ácido nucleico deber ser extraído de forma adecuada de las muestras clínicas. Una forma inadecuada de recolección, almacenaje y/o transporte de las muestras puede dar lugar a falsos negativos.
- Se puede detectar un bajo número de copias molde diana por debajo del límite de detección, pero los resultados pueden no ser reproducibles.



- Existe la posibilidad de falsos positivos debido a la contaminación cruzada con el SARS-CoV-2 ya sea por muestras que contienen altas concentraciones de RNA molde diana o por contaminación por arrastre a partir de productos de PCR de reacciones anteriores.

## 11. Control de calidad

VIASURE SARS-CoV-2 Real Time PCR Detection Kit contiene controles positivo y negativo que deben ser incluidos en cada ensayo para interpretar correctamente los resultados. Además, el control interno (CI) en cada pocillo confirma el correcto funcionamiento de la técnica.

## 12. Características del test

### 12.1. Sensibilidad y especificidad clínica

Se evaluaron 100 muestras respiratorias (frotis nasofaríngeos) de pacientes sintomáticos con sospecha de COVID-19 utilizando VIASURE SARS-CoV-2 Real Time PCR Detection Kit. Estos resultados se compararon con los obtenidos por un método de detección molecular empleado en el centro nacional de referencia (Instituto de Salud Carlos III (ISCIII)). Los resultados fueron los siguientes:

VIASURE SARS-CoV-2 Real Time PCR Detection Kit	Método de detección molecular			Total
		+	-	
	+	2	0	2
-	0	98	98	
Total	2	98	100	

Tabla 6. Comparativa de resultados para SARS-CoV-2.

Además, se realizó otra evaluación clínica del test VIASURE SARS-CoV-2 Real Time PCR Detection Kit con 34 frotis orofaríngeos artificiales recolectados en medios de transporte viral (VTM). Se contaminaron 10 frotis orofaríngeos negativos con RNA de la cepa Human 2019-nCoV BetaCoV/Germany/BavPat1/2020 p.1, y por otro lado se contaminaron otras 12 muestras negativas con concentraciones conocidas de cDNA molde de cada diana. Todas ellas fueron analizadas a ciegas. 33/34 muestras enriquecidas se detectaron correctamente.

Los resultados muestran una alta sensibilidad y especificidad para detectar SARS-CoV-2 utilizando VIASURE SARS-CoV-2 Real Time PCR Detection Kit.

### 12.2. Sensibilidad analítica

VIASURE SARS-CoV-2 Real Time PCR Detection Kit tiene un límite de detección de  $\geq 10$  copias de RNA por reacción para los genes *ORF1ab* y *N* (Figuras 2 y 3).



Figura 2. Diluciones seriadas de un estándar del gen *ORF1ab* ( $10^7$ - $10^1$  copias/reacción). Experimento realizado en el equipo Bio-Rad CFX96™ Real-Time PCR Detection System (canal FAM).


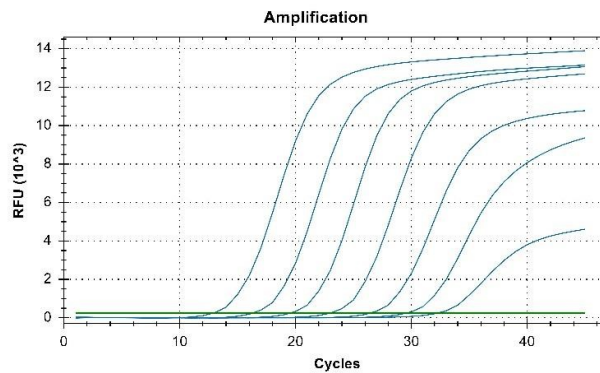


Figura 3. Diluciones seriadas de un estándar del gen N ( $10^7$ - $10^1$  copias/reacción). Experimento realizado en el equipo Bio-Rad CFX96™ Real-Time PCR Detection System (canal ROX).



### 12.3. Especificidad analítica

La especificidad del ensayo del SARS-CoV-2 fue confirmada probando un panel compuesto por diferentes microorganismos que representan los patógenos respiratorios más comunes. No se detectaron reacciones cruzadas con ninguno de los siguientes microorganismos testados, excepto con los patógenos diana que detecta cada ensayo.

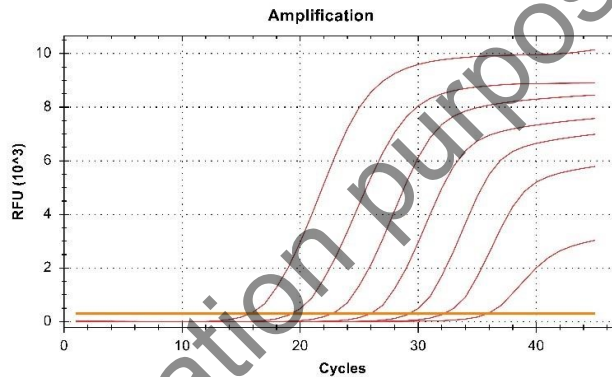

Prueba de reactividad cruzada					
<i>Bordetella pertussis</i>	-	<i>Streptococcus pneumoniae</i> Z022	-	Virus Influenza A/Anhui/1/2013 (H7N9)	-
<i>Bordetella parapertussis</i>	-	<i>Staphylococcus aureus subsp. aureus</i>	-	Virus Influenza B/Brisbane/60/2008	-
<i>Bordetella holmesii</i>	-	<i>Moraxella catarrhalis</i>	-	Virus Influenza B/Florida/04/06	-
<i>Bordetella bronchiseptica</i>	-	<i>Mycobacterium tuberculosis</i> not rifampin resistant	-	Virus Influenza B/Phuket/3073/2013	-
<i>Haemophilus influenzae</i> MinnA	-	<i>Pneumocytis jirovecii</i>	-	Virus Parainfluenza humanos 1, 2, 3 y 4	-
<i>Chlamydia caviae</i>	-	Virus Influenza A/New Caledonia/20/99(H1N1)	-	Virus metapneumovirus humano A y B	-
<i>Chlamydia psittaci</i> genotypes A and C	-	Virus Influenza A/California/7/2009(H1N1)	-	Virus rhinovirus humano tipo C	-
<i>Chlamydomphila pneumoniae</i> CM-1	-	Virus Influenza A/Michigian/45/2015 (H1N1)pdm09	-	Adenovirus Tipo 1-5, 8, 15, 31, 40 y 41	-
<i>Legionella bozemanii</i>	-	Virus Influenza A/Singapore/GP1908/2015 (H1N1)pdm09	-	Bocavirus humano	-
<i>Legionella micdadei</i>	-	Virus Influenza A/Perth/16/2009(H3N2)	-	Virus Respiratorio Sincitial (VRS) A y B	-
<i>Legionella dumoffii</i>	-	Virus Influenza A/Thüringen/5/2017 (H3N2)	-	Coronavirus humano 229E, OC43, NL63 and HKU1	-
<i>Legionella pneumophila</i>	-	Virus Influenza A/Switzerland/9715293/2013 (H3N2)	-	Coronavirus MERS	-
<i>Legionella longbeache</i>	-	Virus Influenza A/Hong Kong/4801/2014(H3N2)	-	SARS Coronavirus Strain Frankfurt 1	-
<i>Mycoplasma pneumoniae</i>	-	Virus Influenza A/DE-SH/Reiherente/AR8444/ 2016 (H5N8)	-		-

Tabla 7. Microorganismos patógenos de referencia utilizados en este estudio.

### 12.4. Reactividad analítica

La reactividad de VIASURE SARS-CoV-2 Real Time PCR Detection Kit se evaluó frente a RNA extraído a partir del virus Human 2019-nCoV cepa BetaCoV/Germany/BavPat1/2020 p.1 mostrando un resultado positivo.











### 13. Bibliography/Bibliografía

- Centers of Disease Control and Prevention (CDC). 2019 Novel Coronavirus, Symptoms. Available from <https://www.cdc.gov/coronavirus/2019-ncov/about/symptoms.html> Accessed February 2020.
- Chen N. *et al.* Epidemiological and Clinical Characteristics of 99 Cases of 2019-Novel Coronavirus (2019-nCoV) Pneumonia in Wuhan, China. *The Lancet*, 2020. DOI: 10.1016/S0140-6736(20)30211-7.
- Huang, C. *et al.* Clinical features of patients infected with 2019 novel coronavirus in Wuhan, China. *The Lancet*, 2020. DOI : 10.1016/S0140-6736(20)30183-5.
- Lu R. *et al.* Genomic characterisation and epidemiology of 2019 novel coronavirus: implications for virus origins and receptor binding. *The Lancet*, 2020. DOI : 10.1016/S0140-6736(20)30251-8.
- Rothe C. *et al.* Transmission of 2019-nCoV Infection from an Asymptomatic Contact in Germany. *New England Journal of Medicine*, 2020. DOI : 10.1056/NEJMc2001468.
- World Health Organization. Global Surveillance for human infection with novel coronavirus (2019-nCoV). Interim guidance v3. 31 January 2020. Available from [https://www.who.int/publications-detail/global-surveillance-for-human-infection-with-novel-coronavirus-\(2019-ncov\)](https://www.who.int/publications-detail/global-surveillance-for-human-infection-with-novel-coronavirus-(2019-ncov)) Accessed February 2020.



7. World Health Organization. Laboratory testing for 2019 novel coronavirus (2019-nCoV) in suspected human cases. Interim guidance. 14 January 2020. Available from <https://www.who.int/publications-detail/laboratory-testing-for-2019-novel-coronavirus-in-suspected-human-cases-20200117> Accessed February 2020.
8. World Health Organization. MERS situation update. December 2019. Available from <http://applications.emro.who.int/docs/EMCSR246E.pdf?ua=1&ua=1> Accessed February 2020.
9. World Health Organization. Novel Coronavirus(2019-nCoV). Situation Report – 14. Data as reported by 3 February 2020. Available from [https://www.who.int/docs/default-source/coronaviruse/situation-reports/20200203-sitrep-14-ncov.pdf?sfvrsn=f7347413\\_2](https://www.who.int/docs/default-source/coronaviruse/situation-reports/20200203-sitrep-14-ncov.pdf?sfvrsn=f7347413_2) Accessed February 2020.
10. World Health Organization. Novel Coronavirus (2019-nCoV) technical guidance: Laboratory testing for 2019-nCoV in humans. Available from <https://www.who.int/emergencies/diseases/novel-coronavirus-2019/technical-guidance/laboratory-guidance> Accessed February 2020.
11. Zhu N. *et al.* A novel coronavirus from patients with pneumonia in China, 2019. *New England Journal of Medicine.*, 2020. DOI : 10.1056/NEJMoa2001017.

## 14. Symbols for IVD components and reagents/Símbolos para reactivos y productos para diagnóstico *in vitro*

 <p><i>In vitro</i> diagnostic device Producto para diagnóstico <i>in vitro</i></p>	 <p>Keep dry Almacenar en lugar seco</p>	 <p>Use by Fecha de caducidad</p>	 <p>Manufacturer Fabricante</p>	 <p>Batch code Número de lote</p>
 <p>Consult instructions for use Consultar las instrucciones de uso</p>	 <p>Temperature limitation Limitación de temperatura</p>	 <p>Contains sufficient for &lt;n&gt; test Contiene &lt;n&gt; test</p>	 <p>Sample diluent Diluyente de muestra</p>	 <p>Catalogue number Número de referencia</p>





## ANEXO 1

## COMPATIBILIDAD DE LOS EQUIPOS A TIEMPO REAL MÁS COMUNES

Las tiras de bajo perfil pueden usarse en todos los termocicladores equipados con un bloque de perfil bajo, como los sistemas listados en la tabla A.1. Las tiras de perfil alto pueden usarse en todos los termocicladores PCR equipados con bloque de perfil alto o normal (high profile), como los sistemas listados en la tabla A.2. Si no encuentra su termociclador en la siguiente lista, por favor póngase en contacto con su proveedor.

Tabla A.1 TERMOCICLADORES CON BLOQUE DE BAJO PERFIL	
Fabricante	Modelo
Agilent Technologies	AriaMx/AriaDx Real-Time PCR System
Applied Biosystems	7500 Fast Real-Time PCR System <sup>(1)</sup>
Applied Biosystems	7500 Fast Dx Real-Time PCR System <sup>(1)</sup>
Applied Biosystems	QuantStudio™ 12K Flex 96-well Fast
Applied Biosystems	QuantStudio™ 6 Flex 96-well Fast
Applied Biosystems	QuantStudio™ 7 Flex 96-well Fast
Applied Biosystems	QuantStudio™ 3 Fast Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	QuantStudio™ 5 Fast Real-Time PCR System
Applied Biosystems	StepOne Plus™ Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	StepOne™ Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	ViiA™ 7 Fast Real-Time PCR System
BIONEER	Exicycler™ 96
Bio-Rad	CFX96™ / CFX96™ IVD Real-Time PCR Detection System
Bio-Rad	Mini Opticon™ Real-Time PCR Detection System <sup>(6)</sup>
Cepheid	SmartCycler® <sup>(3)</sup>
Qiagen	Rotor-Gene® Q <sup>(3)</sup>
Roche	LightCycler® 480 Real-Time PCR System <sup>(4)</sup>
Roche	LightCycler® 96 Real-Time PCR System <sup>(4)</sup>
Roche	Cobas z480 Analyzer <sup>(4)</sup>

(1) Seleccionar Ramp Speed "Standard".

(2) Ver Anexo 3 para la configuración de los valores de exposición.

(3) El producto se debe reconstituir siguiendo el procedimiento adecuado (ver Procedimiento del test) y transvasar a los tubos específicos Rotor-Gene® Q o SmartCycler®.

(4) Se necesita un soporte especial que ajuste con estos equipos Roche de PCR a tiempo real.

(5) No lectura en canal Cy5.

(6) Lectura solo en canales FAM y HEX.

Tabla A1/A2. Equipos compatibles de PCR a tiempo real más comunes.

Tabla A.2 TERMOCICLADORES CON BLOQUE DE PERFIL ALTO	
Fabricante	Modelo
Abbott	Abbott m2000 RealTime System
Applied Biosystems	7300 Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	7500 Real-Time PCR System
Applied Biosystems	7900 HT Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	ABI PRISM 7000 <sup>(6)</sup>
Applied Biosystems	ABI PRISM 7700 <sup>(5)</sup>
Applied Biosystems	QuantStudio™ 12K Flex 96-well
Applied Biosystems	QuantStudio™ 6 Flex 96-well
Applied Biosystems	QuantStudio™ 7 Flex 96-well
Applied Biosystems	QuantStudio™ 3 Real-Time PCR System <sup>(5)</sup>
Applied Biosystems	QuantStudio™ 5 Real-Time PCR System
Applied Biosystems	ViiA™ 7 Real-Time PCR System
Analytik Jena Biometra	TOptical
Analytik Jena Biometra	qTOWER 2.0
BIONEER	Exicycler™ 96
Bio-Rad	CFX96™ / CFX96™ IVD Real-Time PCR Detection System
Bio-Rad	iCycler iQ™ Real-Time PCR Detection System
Bio-Rad	iCycler iQ™5 Real-Time PCR Detection System
Bio-Rad	MyiQ™ Real-Time PCR Detection System <sup>(6)</sup>
Bio-Rad	MyiQ™2 Real-Time PCR Detection System <sup>(6)</sup>
Cepheid	SmartCycler® <sup>(3)</sup>
DNA-Technology	DTprime Real-time Detection Thermal Cycler <sup>(2)</sup>
DNA-Technology	DTlite Real-Time PCR System <sup>(2)</sup>
Eppendorf	Mastercycler™ep realplex
Qiagen	Rotor-Gene® Q <sup>(3)</sup>
Stratagene / Agilent Technologies	Mx3000P™ Real Time PCR System
Stratagene / Agilent Technologies	Mx3005P™ Real Time PCR System



## ANEXO 2

## CANALES DE DETECCIÓN DE LOS EQUIPOS A TIEMPO REAL MÁS COMUNES

Los canales de fluorescencia de algunos de los termocicladores a tiempo real más comunes se especifican en la Tabla A3.

TERMOCICLADORES A TIEMPO REAL	CANAL VIASURE	CANAL DE DETECCIÓN	OBSERVACIONES
Bio-Rad CFX96™	FAM	FAM	Algunos pocillos pueden tener una deriva anormal de la fluorescencia durante los ciclos iniciales de la carrera, dando lugar a una línea ascendente no sigmoidea. Si ve este efecto, en el menú Setting, seleccione la opción Apply Fluorescence Drift Correction dentro de Baseline Settings para corregirlo.
	HEX	HEX	
	ROX	ROX	
	Cy5	Cy5	
ABI 7500 Applied Biosystems	FAM	FAM	Opción del control pasivo ROX desactivada. Algunos pocillos pueden tener una deriva anormal de la fluorescencia durante los ciclos iniciales de la carrera, dando lugar a una línea ascendente no sigmoidea. Si ve este efecto, por favor modifique la línea base (Baseline): Seleccione los valores para Start Cycle y End Cycle de forma que la línea base termine antes de comienzo la detección de un aumento significativo de la fluorescencia.
	HEX	VIC	
	ROX	ROX	
	Cy5	Cy5	
Roche Lightcycler®480II	FAM	465/510	Se requiere compensación de color
	HEX	533/580	
	ROX	533/610	
	Cy5	618/660	
Smartcycler® Cepheid	FAM	Channel 1	
	HEX	Channel 2	
	ROX	Channel 3	
	Cy5	Channel 4	
Abbott m2000rt	FAM	FAM	
	HEX	VIC	
	ROX	ROX	
	Cy5	Cy5	
Mx3000P™ Mx 3005P™ Stratagene	FAM	FAM	Opción del control pasivo ROX desactivada
	HEX	VIC	
	ROX	ROX	
	Cy5	Cy5	
AriaMx Agilent	FAM	FAM	
	HEX	HEX	
	ROX	ROX	
	Cy5	Cy5	
Rotor-Gene®Q Qiagen	FAM	Green	Durante la configuración de los canales (Channel Setup), presione el botón "Gain Optimisation" y después vaya a "Optimise Acquaring". La fluorescencia del apartado Target Sample Range tiene que estar entre 5 y 10 FI para cada canal. Además, marque la opción "Perform Optimisation Before 1st Acquisition".
	HEX	Yellow	
	ROX	Orange	
	Cy5	Red	
Mic Real Time PCR Cycler bms	FAM	Green	En el menú "Run Profile", introduzca los parámetros correctos para "Temperature Control" (Standard TAQ (v3)), Volume (20 ul) y el protocolo térmico apropiado. En la ventana "Cycling", seleccione la opción "Acquire on" para todos los canales haciendo click sobre ellos. Utilice los valores de "Gain" que aparecen por defecto para cada canal (Green = 3, Yellow = 10, Orange = 10, Red = 10).
	HEX	Yellow	
	ROX	Orange	
	Cy5	Red	
Exicycler™ 96 BIONEER	FAM	FAM	
	HEX	JOE	
	ROX	ROX	
	Cy5	Cy5	

Tabla A3: Canales de detección de fluorescencia de diferentes equipos de PCR a Tiempo Real



## ANEXO 3

**CONFIGURACIÓN DE LOS VALORES DE EXPOSICIÓN**

Los parámetros de exposición de algunos termocicladores deben ajustarse para su adecuación y correcto funcionamiento con los test "VIASURE Real Time PCR Detection Kits". Este ensayo ha sido validado con los siguientes valores de exposición:

- DTprime Real-time Detection Thermal Cyclers (DNA-Technology): canal FAM -500\*, canal HEX - 1000, canal ROX - 1000 y canal Cy5 -1000.

- DTlite Real-Time PCR System (DNA-Technology): canal FAM -500, canal HEX - 500, canal ROX - 500 y canal Cy5 - 500.

\*Si el resultado en el canal FAM no es el esperado, no hay amplificaciones o se observa elevado ruido de fondo, por favor, baje los valores de exposición indicados anteriormente hasta 150.

For information purposes only



- CFX™ and IQ5™ are registered trademarks of Bio-Rad Laboratories.
- ABI®, QuantStudio™, StepOnePlus™ and ViiA™ are registered trademarks of Thermo Fisher Scientific Inc.
- LightCycler® is a registered trademark of Roche.
- Mx3000P™, Mx3005™ and AriaMx are registered trademarks of Agilent Technologies.
- Mastercycler™ is a registered trademark of Eppendorf.
- Rotor-Gene®Q is a registered trademark of Qiagen.
- SmartCycler® is a registered trademark of Cepheid.

Revision: March 2020

For information purposes only



For information purposes only



**CerTest Biotec, S.L.**

Pol. Industrial Río Gállego II · Calle J, Nº1  
50840, San Mateo de Gállego, Zaragoza (Spain)  
www.certest.es



VIASURE online

F-362 rev01

VIASURE



Real Time PCR Detection Kits

CerTest  
BIOTEC