




REFERENCES:

1. van Dongen JJM, et al. EuroFlow-Based Flowcytometric Diagnostic Screening and Classification of Primary Immunodeficiencies of the Lymphoid System. Front. Immunol. 2019 Jun; 10:1271.
2. van der Burg M, et al. The EuroFlow PID Orientation Tube for Flow Cytometric Diagnostic Screening of Primary Immunodeficiencies of the Lymphoid System. Front. Immunol. 2019 Mar; 10:246.
3. Linskens E, et al. Improved Standardization of Flow Cytometry Diagnostic Screening of Primary Immunodeficiency by Software-Based Automated Gating. Front. Immunol. 2020 Nov; 11:584646.
4. Blanco E, et al. Age-associated distribution of normal B-cell and plasma cell subsets in peripheral blood. Journal of Allergy and Clinical Immunology. 2018 Jun; 141(6).
5. Blanco E, et al. Defects in memory B-cell and plasma cell subsets expressing different immunoglobulin-subclasses in patients with CVID and immunoglobulin subclass deficiencies. Journal of Allergy and Clinical Immunology. 2019 Sep; 144(3):809-24.
6. Kalina T, et al. EuroFlow Standardized Approach to Diagnostic Immunophenotyping of Severe PID in Newborns and Young Children. Front. Immunol. 2020 Mar; 11:371.

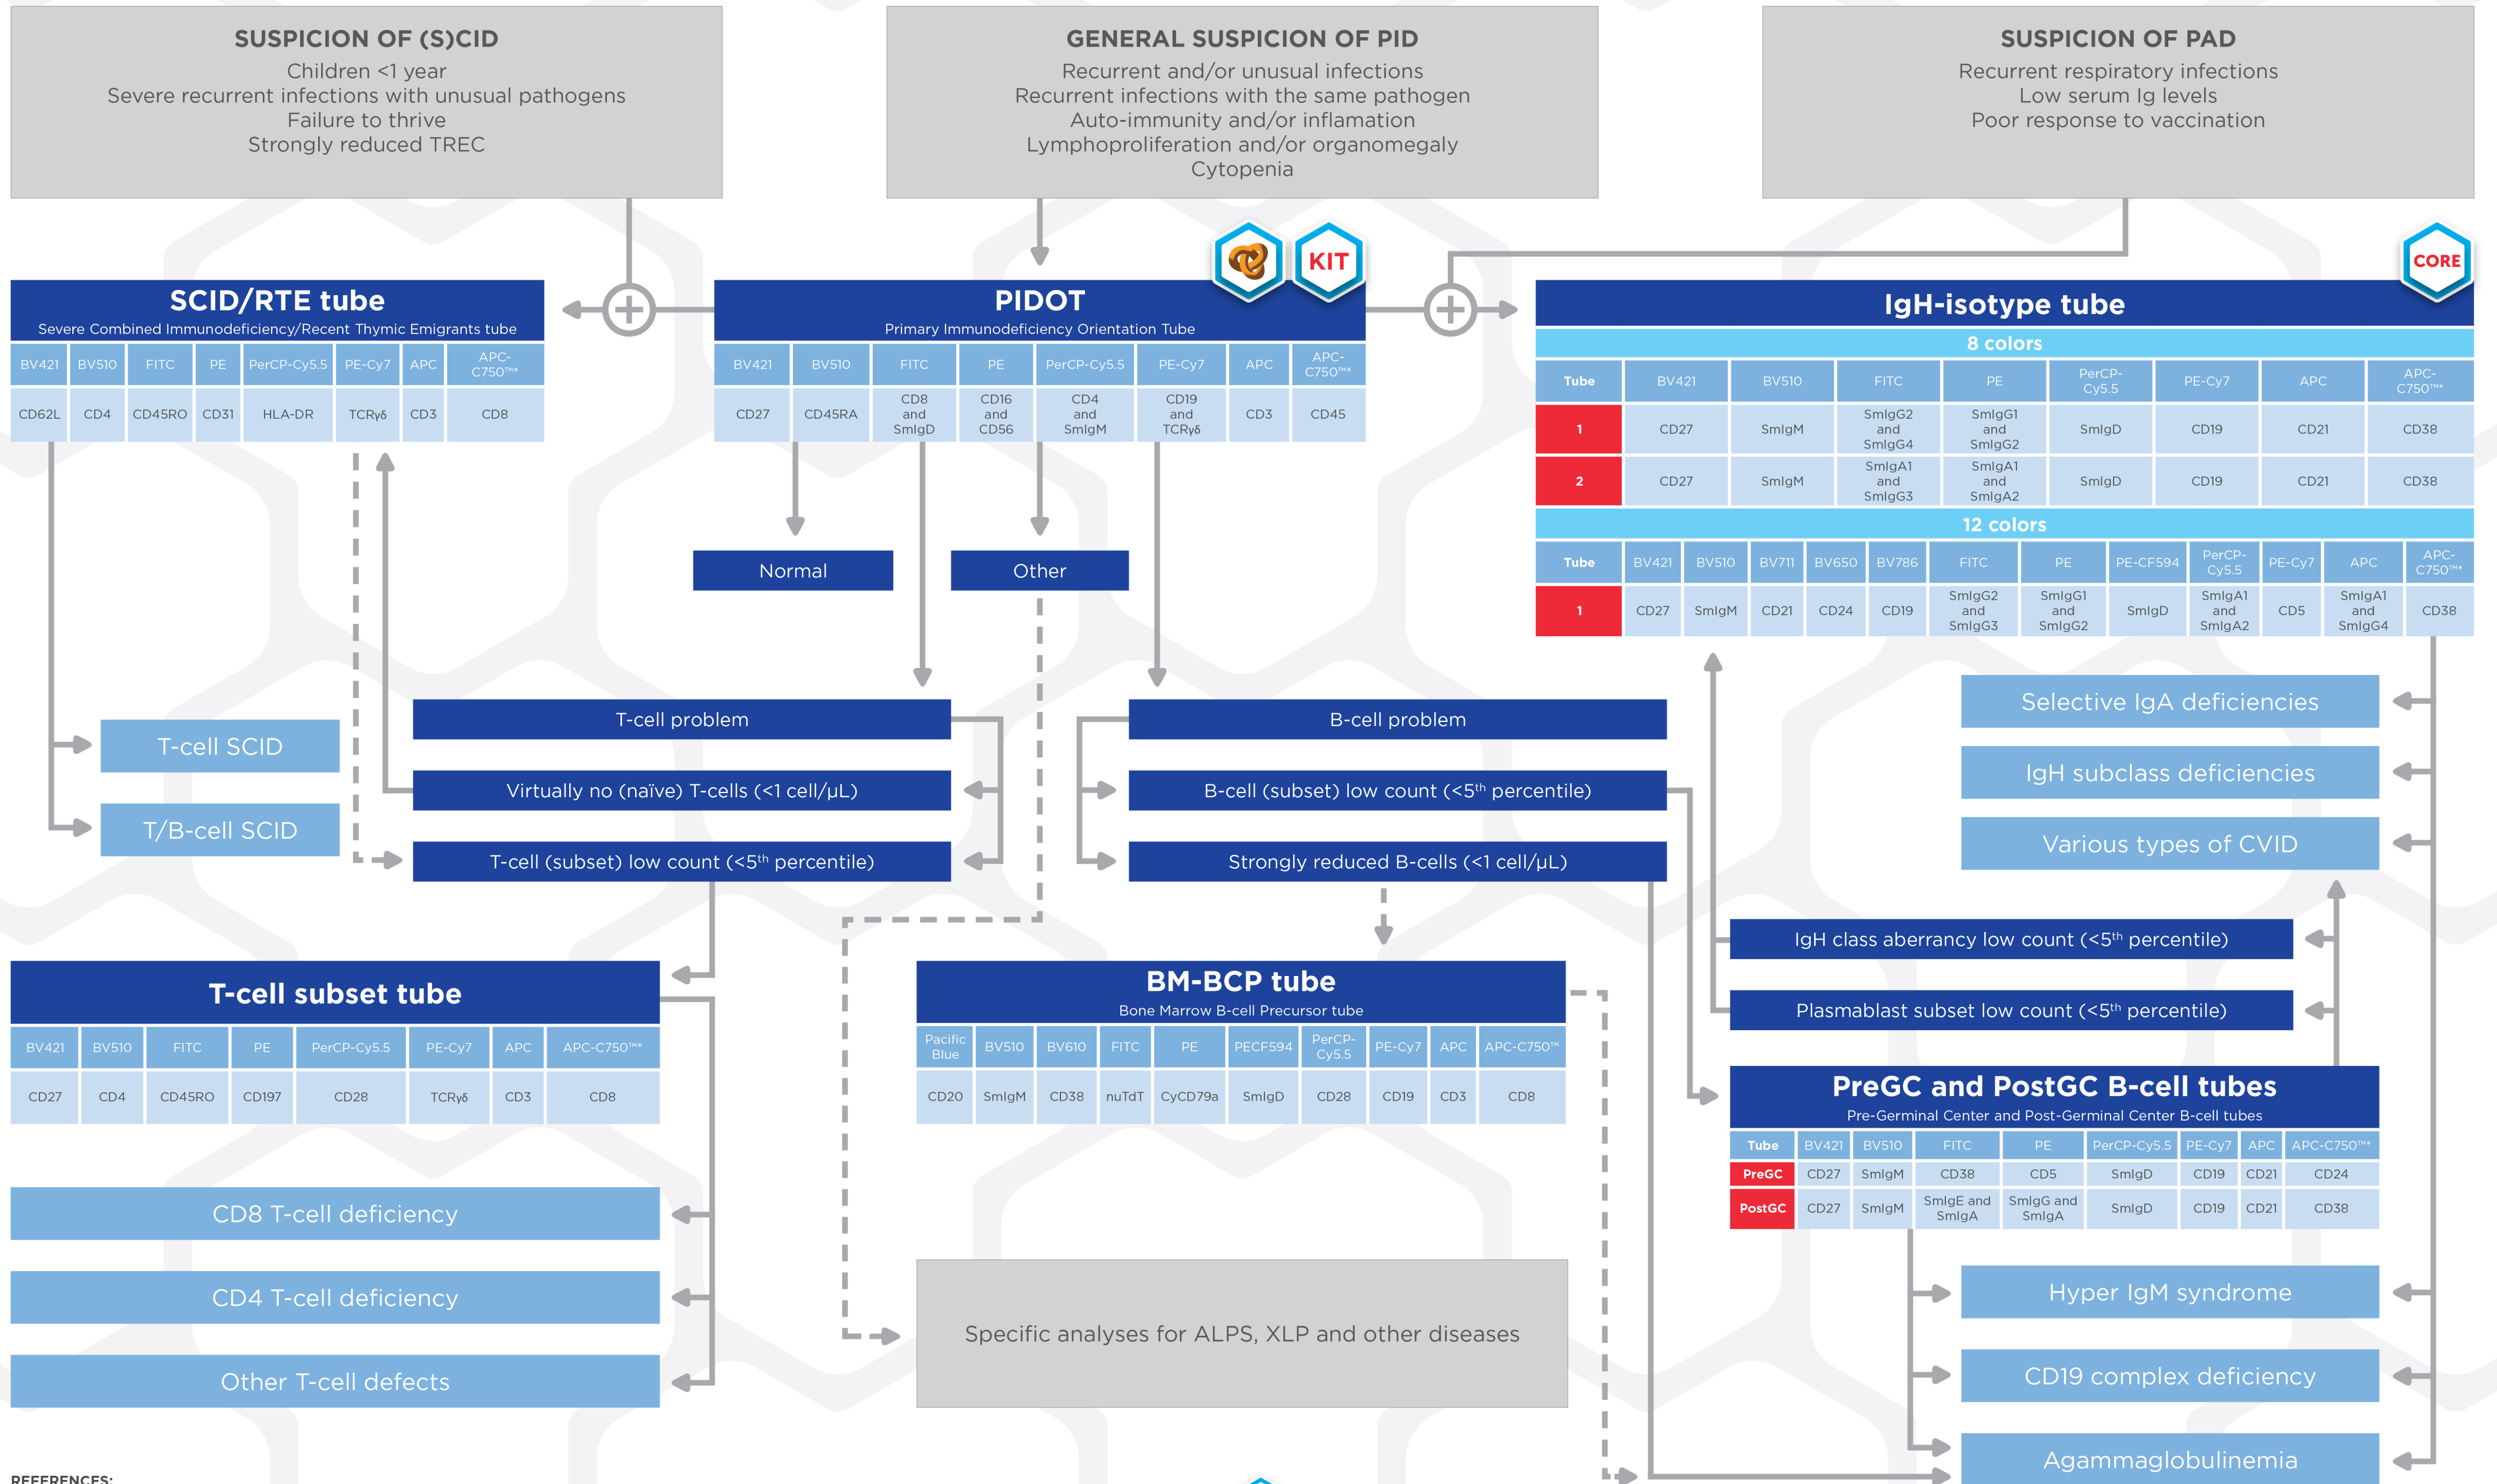

PIDOT (ref. CYT-PIDOT)



IgH-isotype panel - subclasses (1 tube) (ref. (CYT-IGS-1),
IgH-isotype panel - subclasses (2 tubes) (ref. (CYT-IGS-2))



EuroFlow™ databases available in Infinicyt™ for PIDOT

Cytognos offers antibodies and pre-mixed combinations according to EuroFlow™ guidelines.
* Or equivalent fluorochrome

www.cytognos.com | www.euroflow.org

Distributed by Abacus dx

1800 ABACUS (AUS) 0800 222 170 (NZ) | info@abacusdx.com | www.abacusdx.com

abacus dx